
Product Manual


ATP Assay Kit

Catalog Number

MET-5163

100 assays

FOR RESEARCH USE ONLY
Not for use in diagnostic procedures



CELL BIOLABS, INC.

Creating Solutions for Life Science Research

Introduction

Adenosine triphosphate (ATP) is an organic molecule that provides energy for various cell processes such as enzymatic reactions leading to nerve impulses, muscle contraction, and synthesis of chemicals. ATP is found in all life forms and is classified as a nucleoside triphosphate consisting of three components: a nitrogenous base (adenine), the sugar ribose, and the triphosphate group. It is produced in animals from serial enzymatic reactions such as glycolysis or oxidative phosphorylation. In plants, sunlight is converted into ATP through a process known as photosynthesis. When used up metabolically, ATP is converted either to adenosine diphosphate (ADP) or to adenosine monophosphate (AMP). Other enzymatic reactions occur to regenerate ATP (which is also a precursor to DNA and RNA) and additionally ATP is used as a coenzyme.

Cell Biolabs' ATP Assay Kit is a simple fluorometric assay that measures the amount of total ATP present in biological samples in a 96-well microtiter plate format. Each kit provides sufficient reagents to perform up to 100 assays*, including blanks, ATP standards, and unknown samples. Sample ATP concentrations are determined by comparison with a known ATP standard. The kit has a detection sensitivity limit of 1.56 μM ATP.

**Note: Each sample replicate requires 2 assays, one treated with Glycerol Kinase (+GK) and one without (-GK). ATP is calculated from the difference in RFU readings from the 2 wells.*

Assay Principle

Cell Biolabs' ATP Assay Kit measures total ATP within biological samples. ATP and glycerol are converted by glycerol kinase to ADP and glycerol-3-phosphate. Glycerol-3-phosphate and oxygen are then converted by glycerol-3-phosphate oxidase to glycerone phosphate and hydrogen peroxide. The resulting hydrogen peroxide is then detected with a highly specific fluorometric probe. Horseradish peroxidase catalyzes the reaction between the probe and hydrogen peroxide, which bind in a 1:1 ratio. Samples are compared to a known concentration of ATP standard within the 96-well microtiter plate format. Samples and standards are incubated for 30 minutes and then read with a standard 96-well fluorometric plate reader (Figure 1).

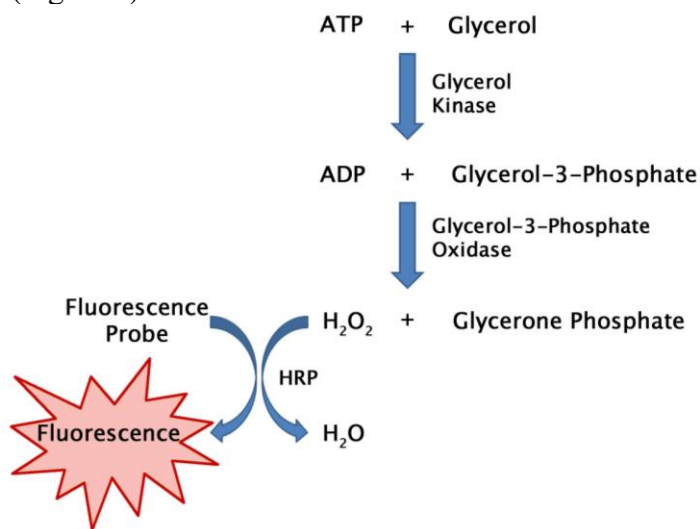


Figure 1. ATP Assay Principle

Related Products

1. MET-5164: ADP Assay Kit
2. MET-5158: Methionine Assay Kit
3. MET-5152: s-Adenosylmethionine ELISA Kit
4. MET-5151: s-Adenosylhomocysteine ELISA Kit
5. MET-5029: Pyruvate Assay Kit (Fluorometric)

Kit Components

Box 1 (shipped on blue ice packs)

1. ATP Standard (Part No. 51631C): One 50 μ L tube at 10 mM.
2. Glycerol Kinase (Part No 51632D): One 330 μ L tube at 15.2 U/mL.
3. Glycerol-3-Phosphate Oxidase (Part No. 51635D): One 610 μ L tube at 37 U/mL.
4. Fluorometric Probe (Part No. 50231C): One 50 μ L tube in DMSO.
5. HRP (Part No. 234402-T): One 10 μ L tube of a 100 U/mL solution in glycerol.

Box 2 (shipped on blue ice packs)

1. Neutralization Buffer (Part No. 51634A): One 25 mL bottle.
2. 10X Assay Buffer (Part No. 51633A): One 25 mL bottle.

Materials Not Supplied

1. Distilled or deionized water
2. 10 kDa molecular weight cutoff (MWCO) centrifuge spin filter (e.g. Amicon Ultra 0.5mL)
3. Standard 96-well fluorescence black microtiter plate and/or black cell culture microplate
4. Concentrated perchloric acid

Storage

Store the 10X Assay Buffer and Neutralization Buffer at room temperature. Store the Glycerokinase and the Glycerol-3-Phosphate Oxidase at -80°C . Store all other components at -20°C . The Fluorometric Probe is light sensitive and must be stored accordingly. Avoid multiple freeze/thaw cycles.

Preparation of Reagents

- 1X Assay Buffer: Dilute the 10X Assay Buffer 1:10 with deionized water for a 1X solution. Stir or vortex to homogeneity. Store at 4°C .
- Reaction Mix and Negative Control Mix: Prepare two separate mixtures according to the table below. The Glycerol kinase is omitted from the Negative Control Mix.

Component	Reaction Mix (20 assays)	Negative Control Mix (20 assays)
Glycerol kinase	66 μ L	-----
Glycerol-3-Phosphate Oxidase	122 μ L	122 μ L
HRP	2 μ L	2 μ L
Fluorometric Probe	10 μ L	10 μ L
1X Assay Buffer	800 μ L	866 μ L
Total	1000 μL	1000 μL

Note: Prepare only enough for immediate use and scale proportionally as needed.

- 0.5 M Perchloric Acid: Dilute concentrated perchloric acid (not provided in the kit) to 0.5 M with distilled water. Store at room temperature.

Preparation of Samples

- Cell culture supernatants: To remove insoluble particles, centrifuge at 10,000 rpm for 5 min. Collect the supernatant and filter the solution with a 10 kDa spin filter to deproteinate the sample. Collect flow through. The flow through may be assayed directly or diluted as necessary into 1X Assay Buffer.
Note: Maintain pH between 7 and 8 for optimal working conditions as the Fluorometric Probe is unstable at high pH (>8.5).
- Tissue lysates: Sonicate or homogenize 150-300 milligrams of tissue sample in 2 mL of 0.5 M Perchloric Acid at 4°C. Incubate for 5 minutes at 4°C. Centrifuge at 18000 x g for 5 minutes. Collect the supernatant and transfer to a new tube. Add 500 μ L of Neutralization Buffer and mix well. Incubate for 5 minutes at 4°C. Centrifuge at 18000 x g for 5 minutes. Collect the supernatant and transfer to a new tube. Store aliquots at -80°C until ready to use. *Upon thawing, if salt crystals are observed, warm the sample to 37°C for 5 minutes and vortex well to resuspend.*
- Cell lysates: Wash cells in PBS and transfer to an Eppendorf tube. Centrifuge 1.5×10^7 cells at 1000 x g for 5 minutes. Remove the supernatant and resuspend cell pellet in 200 μ L of 0.5 M Perchloric Acid. Incubate for 5 minutes at 4°C. Centrifuge at 18000 x g for 5 minutes. Collect the supernatant and transfer to a new tube. Add 50 μ L of Neutralization Buffer and mix well. Incubate for 5 minutes at 4°C. Centrifuge at 18000 x g for 5 minutes. Collect the supernatant and transfer to a new tube. Store aliquots at -80°C until ready to use. *Upon thawing, if salt crystals are observed, warm the sample to 37°C for 5 minutes and vortex well to resuspend.*
- Serum, plasma, saliva, or urine: To remove insoluble particles, centrifuge at 10,000 rpm for 5 min. Collect the supernatant and filter the solution with a 10 kDa spin filter to deproteinate the sample. Collect flow through. The flow through may be assayed directly or diluted as necessary into 1X Assay Buffer.

Notes:

- *All samples should be assayed immediately or stored at -80°C for up to 1-2 months. Run proper controls as necessary. Optimal experimental conditions for samples must be determined by the investigator. Always run a standard curve with samples.*
- *Samples with NADH concentrations above 10 μ M and glutathione concentrations above 50 μ M will oxidize the Fluorometric Probe and could result in erroneous readings. To minimize this interference, it is recommended that superoxide dismutase (SOD) be added to the reaction at a final concentration of 40 U/mL (Votyakova and Reynolds, Ref. 2).*

- Avoid samples containing DTT or β -mercaptoethanol since the Fluorometric Probe is not stable in the presence of thiols (above 10 μ M).

Preparation of Standard Curve

Prepare fresh ATP standards by diluting in distilled water according to Table 1.

Standard Tubes	10 mM ATP Solution (μ L)	Water (μ L)	ATP (μ M)
1	5	495	100
2	250 of Tube #1	250	50
3	250 of Tube #2	250	25
4	250 of Tube #3	250	12.5
5	250 of Tube #4	250	6.25
6	250 of Tube #5	250	3.123
7	250 of Tube #6	250	1.56
8	0	250	0

Table 1. Preparation of ATP Standards.

Assay Protocol

1. Prepare and mix all reagents thoroughly before use. Each sample, including unknowns and standards, should be assayed in duplicate or triplicate.
Note: Each unknown sample replicate requires two paired wells, one to be treated with Glycerokinase (+GK) and one without the enzyme (-GK) to measure endogenous background.
2. Add 50 μ L of each ATP standard or unknown sample into wells of a 96-well microtiter plate.
3. Add 50 μ L of Reaction Mix to the standards and to one half of the paired sample wells, and mix the well contents thoroughly.
4. Add 50 μ L of Negative Control Mix to the other half of the paired sample wells.
5. Mix the well contents thoroughly and incubate for 30 minutes at 37°C protected from light.
Note: This assay is continuous (not terminated) and therefore may be measured at multiple time points to follow the reaction kinetics.
6. Read the plate with a fluorescence microplate reader equipped for excitation in the 530-570 nm range and for emission in the 590-600 nm range.

Example of Results

The following figures demonstrate typical ATP Assay Kit results. One should use the data below for reference only. This data should not be used to interpret or calculate actual sample results.

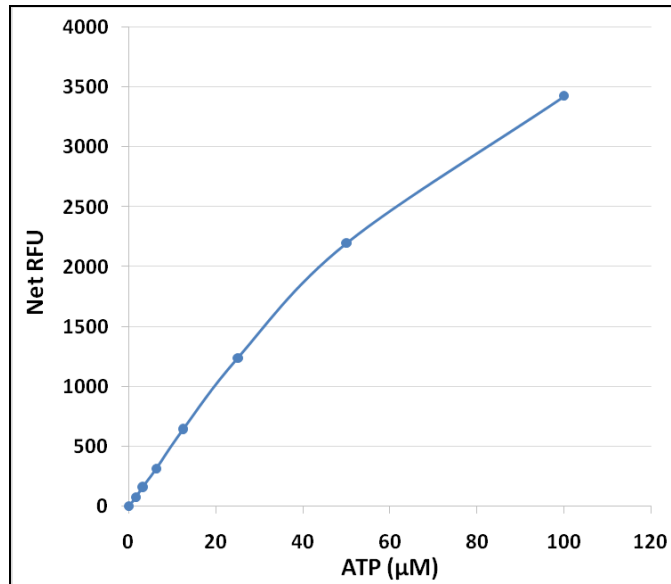


Figure 2: ATP Standard Curve.

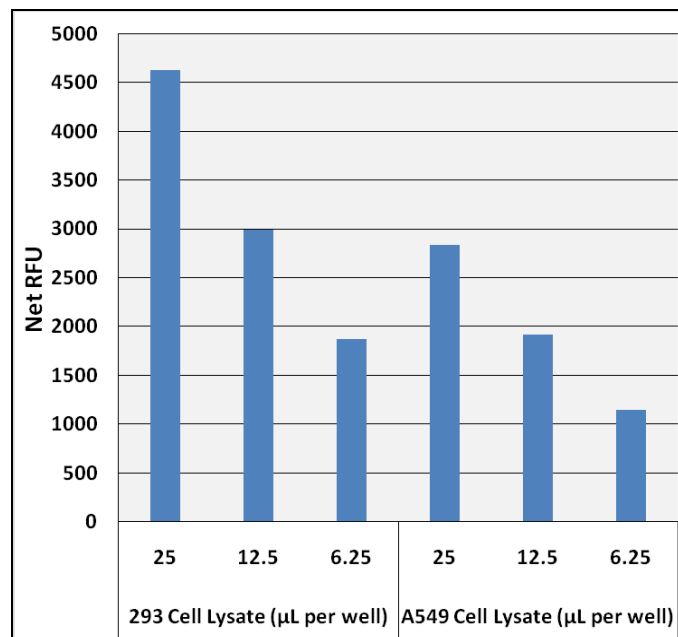


Figure 3: ATP Detection in 293 and A549 cells using the ATP Assay Kit. Cell lysates were prepared according to the preparation of samples section above.

Calculation of Results

1. Determine the average Relative Fluorescence Unit (RFU) values for each sample, control, and standard.
2. Subtract the average zero standard value from itself and all standard values.
3. Graph the standard curve (see Figure 2).

4. Subtract the sample well values without Glycerol kinase (-GK) from the sample well values containing Glycerol kinase (+GK) to obtain the difference. The fluorescence difference is due to the Glycerol kinase activity.

$$\text{Net RFU} = (\text{RFU}_{+\text{GK}}) - (\text{RFU}_{-\text{GK}})$$

5. Compare the net RFU of each sample to the standard curve to determine and extrapolate the quantity of ATP present in the sample. Only use values within the range of the standard curve.

References

1. Knowles J R (1980) *Annu. Rev. Biochem.* **49**: 877–919.
2. Votyakova TV, and Reynolds IJ (2001) *Neurochem.* **79**:266.
3. Törnroth-Horsefield S and Neutze R. (2008). *Proc Natl Acad Sci USA.* **105**: 19565–19566.
4. Feng L-L, Cai Y-Q, Zhu M-C, Xing L-J, and Wang X (2020) *Cancer Cell Int* 20: 110
5. Watt IN, Montgomery MG, Runswick MJ, Leslie AGW, and Walker JE (2010) *Proc Natl Acad Sci USA* **107**:16823-16827

Recent Product Citation

Tan, L. et al. (2024). The New Nano-Resuscitation Solution (TPP-MR) Attenuated Myocardial Injury in Hemorrhagic Shock Rats by Inhibiting Ferroptosis. *Int J Nanomedicine.* **19**:7567-7583. doi: 10.2147/IJN.S463121.

Warranty

These products are warranted to perform as described in their labeling and in Cell Biolabs literature when used in accordance with their instructions. THERE ARE NO WARRANTIES THAT EXTEND BEYOND THIS EXPRESSED WARRANTY AND CELL BIOLABS DISCLAIMS ANY IMPLIED WARRANTY OF MERCHANTABILITY OR WARRANTY OF FITNESS FOR PARTICULAR PURPOSE. CELL BIOLABS's sole obligation and purchaser's exclusive remedy for breach of this warranty shall be, at the option of CELL BIOLABS, to repair or replace the products. In no event shall CELL BIOLABS be liable for any proximate, incidental or consequential damages in connection with the products.

Contact Information

Cell Biolabs, Inc.
5628 Copley Drive
San Diego, CA 92111
Worldwide: +1 858 271-6500
USA Toll-Free: 1-888-CBL-0505
E-mail: tech@cellbiolabs.com
www.cellbiolabs.com

©2023-2025: Cell Biolabs, Inc. - All rights reserved. No part of these works may be reproduced in any form without permissions in writing.